

HAMILTON, BROOK, SMITH & REYNOLDS, P.C.

UTILITY PATENT APPLICATION TRANSMITTAL <small>(Only for new nonprovisional applications under 37 C.F.R. 1.53(b))</small>	Attorney Docket No.	2506.1013-001
	First Named Inventor or Application Identifier	Derek D. Mahoney
	Express Mail Label No.	EL192649211US

JCS30 U.S. PTO
 09/524040
 03/13/00

A

Title of Invention	ONE-SIZE-FITS-ALL UNI-EAR HEARING INSTRUMENT
--------------------	--

APPLICATION ELEMENTS See MPEP chapter 600 concerning utility patent application contents.	ADDRESS TO: Assistant Commissioner for Patents Box Patent Application Washington, D.C. 20231
---	---

1. <input type="checkbox"/> Fee Transmittal Form <i>(Submit an original, and a duplicate for fee processing)</i> 2. <input checked="" type="checkbox"/> Specification [Total Pages [19]] <i>(preferred arrangement set forth below)</i> - Descriptive title of the invention - Cross References to Related Applications - Statement Regarding Fed sponsored R & D - Reference to microfiche Appendix - Background of the Invention - Summary of the Invention - Brief Description of the Drawings - Detailed Description - Claim(s) - Abstract of the Disclosure 3. <input checked="" type="checkbox"/> Drawing(s) (35 U.S.C. 113) [Total Sheets [5]] <input type="checkbox"/> Formal <input checked="" type="checkbox"/> Informal 4. <input type="checkbox"/> Oath or Declaration/POA [Total Pages []] a. <input type="checkbox"/> Newly executed (original or copy) b. <input type="checkbox"/> Copy from a prior application (37 C.F.R. 1.63(d)) <i>(for continuation/divisional with Box 17 completed)</i> [NOTE Box 5 below] i. <input type="checkbox"/> <u>DELETION OF INVENTOR(S)</u> Signed statement attached deleting inventor(s) named in the prior application, see 37 C.F.R. 1.63(d)(2) and 1.33(b). 5. <input type="checkbox"/> Incorporation By Reference <i>(useable if Box 4b is checked)</i> The entire disclosure of the prior application, from which a copy of the oath or declaration is supplied under Box 4b, is considered as being part of the disclosure of the accompanying application and is hereby incorporated by reference therein.	6. <input type="checkbox"/> Microfiche Computer Program <i>(Appendix)</i> 7. <input type="checkbox"/> Nucleotide and/or Amino Acid Sequence Submission <i>(if applicable, all necessary)</i> a. <input type="checkbox"/> Computer Readable Copy b. <input type="checkbox"/> Paper Copy (identical to computer copy) [] Pages c. <input type="checkbox"/> Statement verifying identity of above copies <div style="border: 1px solid black; padding: 5px; margin-top: 10px;"> ACCOMPANYING APPLICATION PARTS 8. <input type="checkbox"/> Assignment Papers (cover sheet & documents) 9. <input type="checkbox"/> 37 C.F.R. 3.73(b) Statement <input type="checkbox"/> Power of Attorney <i>(when there is an assignee)</i> 10. <input type="checkbox"/> English Translation Document <i>(if applicable)</i> 11. <input type="checkbox"/> Information Disclosure Statement (IDS)/PTO-1449 <input type="checkbox"/> Copies of IDS Citations 12. <input type="checkbox"/> Preliminary Amendment 13. <input checked="" type="checkbox"/> Return Receipt Postcard (MPEP 503) <i>(Should be specifically itemized)</i> 14. <input type="checkbox"/> Small Entity Statement(s) <input type="checkbox"/> Statement filed in prior application, status still proper and desired 15. <input type="checkbox"/> Certified Copy of Priority Document(s) <i>(if foreign priority is claimed)</i> 16. <input type="checkbox"/> Other: _____ </div>
---	--

17. If a CONTINUING APPLICATION , check appropriate box and supply the requisite information: <input type="checkbox"/> Continuation <input type="checkbox"/> Divisional <input type="checkbox"/> Continuation-in-part (CIP) of prior application No.: Prior application information: Examiner: Group Art Unit:	
---	--

18. CORRESPONDENCE ADDRESS					
NAME	Leo R. Reynolds, Esq.				
	HAMILTON, BROOK, SMITH & REYNOLDS, P.C.				
ADDRESS	Two Militia Drive				
CITY	Lexington	STATE	MA	ZIP CODE	02421-4799
COUNTRY	USA	TELEPHONE	(781) 861-6240	FAX	(781) 861-9540

Signature		Date	3/13/00
Submitted by Typed or Printed Name	Leo R. Reynolds, Esq.	Reg. Number	20,884

03/13/00

JCS30 U.S. PTO

009524040-00000000

LRR/jk
03/13/00

-1-

Date: <u>3/13/00</u>	Express Mail Label No. <u>EL192649211US</u>
----------------------	---

Inventors: Derek D. Mahoney, Walter P. Sjursen, Wayne P. Staab
and Marvin Leedom

Attorney's Docket No.: 2506.1013-001

ONE-SIZE-FITS-ALL UNI-EAR HEARING INSTRUMENT

RELATED APPLICATION

This application claims the benefit under 35 U.S.C. 119(e) of U.S. Provisional Application No. 60/145,410 (Attorney Docket No. SMI-13623p), filed July 23, 1999,
5 the entire teachings of which are incorporated herein by reference.

This application is related to copending U.S. Applications:

ATTORNEY DOCKET NO..	TITLE
SMI-13459pA	Disposable Modular Hearing Aid
2506.1005-001	Mass Produced Hearing Aid With a Limited Set of Acoustical Formats
10 2506.2008-001	Hearing Aid
2506.2012-000	Hearing Aid With Flexible Shell
2506.2013-000	Hearing Aid Prescription Selector
2506.2014-000	Through-Hole and Surface Mount Technologies for Highly-Automatable Hearing Aid Receivers
2506.2019-000	Remote Programming and Control Means for a Hearing Aid

15 all filed of even date herewith, the entire teachings of which are incorporated herein by reference.

BACKGROUND OF THE INVENTION

The invention herein generally relates to a miniature electroacoustic instrument and, in particular, a peritympanic hearing instrument suitable for use in humans.

Hearing instruments typically are custom-designed to suit the anatomical and
5 audiological needs of an individual user. Because custom-made devices can be very
costly, it is desirable to mass-produce a hearing instrument that is relatively inexpensive
and is readily adaptable to most users' anatomical and audiological requirements, and
which is inconspicuous and lightweight.

There are significant challenges associated with the development of mass-
10 produced hearing instruments. Although the structure of the external auditory canal
generally is a sinuous, oval cylinder with three sections, it can vary significantly
depending on the particular individual. Traversing the outer canal towards the inner
tympanic membrane, the first section is directed inward, forward, and slightly upward.
The next section tends to pass inward and backward. The final section is carried
15 inward, forward, and slightly downward. The outer portion of the ear canal is
surrounded by cartilaginous tissue, with the inner portion being surrounded by bone.
The canal is formed with a very thin lining of skin, which is extremely sensitive to the
presence of foreign objects. Further details of the path and contours of the external
auditory canal are described in U.S. Patent No. 4,870,688, issued to Barry Voroba et al.,
20 and in U.S. Patent No. 5,701,348, issued to Adnan Shennib, both of which are
incorporated herein by reference.

U.S. Patent No. 4,870,688 describes an in-the-canal miniaturized hearing aid
contained within a prefabricated ear shell assembly composed of a hollow rigid body
with a soft, resilient covering fixed to its exterior. The microphone, receiver, amplifier,
25 and battery are all wholly contained within a prefabricated modular sound assembly
which snaps into a patient-selectable prefabricated ear shell assembly. The soft,
resilient covering that is affixed to the exterior of the rigid core is intended to allow the
cylindrical or elliptical shape of the in-the-canal hearing aid to more easily conform to
the individual variations in a user's auditory canal.

U.S. Patent No. 5,701,348 described a hearing device having highly articulated, non-contiguous parts including a receiver module for delivering acoustic signals, a main module containing all of the hearing aid components except the receiver, and a connector that is articulated with both the receiver module and the main module to permit independent movement of the receiver and main modules. Separation of the receiver from the main module, and the receiver's articulation with respect to the main module, is intended to provide at least two degrees of freedom in movement and independent movement of the receiver module with respect to the main module, and visa versa.

Attempts have also been made to provide inserts intended to be used as a part of a hearing aid device. U.S. Patent No. 2,487,038, issued to Jasper Baum, describes an ear insert shaped for insertion into the concha or the outer cavity of an ear. It includes a series of ball-shaped ball-like wall sections each made with sufficiently thick walls so as to give them great stiffness and prevent substantial distortion of the cross-section of the sound-passage portions extending therethrough under the action of external bending forces when the insert is inserted into the curved space of the outer ear cavity. The ball-like wall sections are interconnected by short neck-like sections to readily flex and take up substantially the entire deformation to which the channel insert is subjected. Thin flexible, skirt-like protrusions in outward and rearward directions from the ball-like wall sections to become wedged against the surrounding surface portions of the outer ear cavity for automatically establishing therewith an acoustic seal.

U.S. Patent No. 3,080,011, issued to John D. Henderson, describes an ear canal insert with a very soft tip with flanges. A flexible mounting tube is considerably stiffer than the material of which the head portion flanges are formed so that it can be used to force the insert portion of the device into the ear canal.

U.S. Patent No. 5,201,007, issued to Gary L. Ward et al., describes earmolds that convey amplified sound from the hearing aid to the ear. An acoustic conduction tube extends into the ear canal and a flanged tip on the conduction tube creates a resonant cavity between the tip and the tympanic membrane. The tip is constructed of a flexible

material to form a sealed cavity adjacent the tympanic membrane, permit the seal to be obtained with only slight pressure against the wall of the ear canal, and permit the tip to be oscillated by the natural, unamplified sounds which arrive by air conduction through the ear canal, so that the oscillation can raise the resonant frequencies of the cavity.

- 5 U.S. Patent No. 5,185,802, issued to Mark F. Stanton, describes a modular hearing aid system comprising a customized exterior shell formed of compliant material, in situ, in the usual manner in accordance with the shape of the ear canal of the individual user, such that a separate and distinct shell is required for each ear. A housing containing the hearing aid components is removably inserted in the shell. The
10 housing has a bilateral standardized shape so it can be used with either a right or left ear customized shell.

SUMMARY OF THE INVENTION

- Despite numerous attempts including those described above, there remains a need for a mass-produced hearing instrument that is relatively inexpensive, readily
15 adaptable to an individual's anatomical and audiological requirements, and that is inconspicuous and lightweight. It has been discovered that the development of a prosthetic device that occupies the region traditionally filled by an in-the-canal (ITC) or completing in-the-canal (CIC) device, as well as extending significantly into the peritympanic region, is improbable at best without a device that will allow deep
20 penetration into the ear canal by the hearing instrument. Current "one-size-fits-all" hearing instruments are either of the in-the-ear (ITE) or ITC or CIC variety. Some have the ability to accommodate the first bend in the ear canal. However, conventional hearing instruments fail to adequately and simultaneously accommodate the first and second bends of a typical ear canal and are generally not capable of comfortably
25 extending significantly into the peritympanic region.

Copending U.S. Application Serial No. 09/105,729 entitled "Peritympanic Hearing Instrument" filed June 26, 1998 (Attorney Docket No. SMI-12798) and incorporated herein in its entirety by reference attempts to fulfill many of the

requirements for an acceptable “one-size-fits-all” hearing aid. The referenced application discloses a hearing instrument that is positionable in the external auditory canal of a human at a location that is proximal to the tympanic membrane. The instrument includes a substantially rigid shell that is shaped to enclose a microphone, electronics, as well as a receiver with a distal end portion that faces the tympanic membrane. The instrument is provided with a flexible tip member that is connected adjacent to the distal end portion of the shell.

Like the above referenced copending application, the present invention provides a functional hearing aid body with a suitable shape capable of being located proximately adjacent the tympanic membrane and within the inner canal. However, the shape is formed so that not only is the body capable of being comfortably inserted and left in position in the ear of a “typical user” such that “one-size-fits-all” but one size also fits either the left or right ear, i.e. a “uni-ear” or “non-specific” hearing aid device. Moreover, there is no need to customize the outer shell or to provide a soft compliant, in situ, formed outer mold around the shell.

Note: For purposes of this application, a “typical user” is considered to be a person whose inner canal profile conforms substantially to a profile determined by obtaining impressions from a statistically valid population of potential users.

In addition, a method and apparatus is provided for forming such a structure which includes “inter alia” the following procedures:

First, a plurality of sample ear impressions are taken from the general populace. Next, topological data is generated from the ear impressions. This can be accomplished by well-known three-dimensional scanning, cross-sectioning or a similar technology. The data is then processed using generally a available solid modeling software packages to mathematically generate volume dimensions representing the ear impressions. Next, the dimensions are properly oriented and aligned by the software user and a single new set of volume dimensions is created which represents the intersection of all the sampled impressions. This single new set of volume dimensions is then manipulated using the software to smooth and truncate the shape so as to produce a “one-size-fits-all” shape

(either the left or right ear shape but not both). Next, a mirror image of the one-size-fits-all shape is generated to produce a “mirror image” shape. Data representing the original and mirror image shapes or volumes is then processed as above to create a uni-shape which after minor smoothing and radiusing operations produces a mold for a

5 “uni-ear” hearing aid device.

Preferably, the mold is used to produce two shell halves with interior cores for housing the essential hearing aid parts, such as, the microphone, electronics, battery and speaker (receiver). In addition, the molded body is adapted to retain a soft tip at an appropriate angle proximal to the tympanic membrane. This tip couples sound from the

10 hearing aid receiver to the tympanic membrane and also serves to enhance retention of the hearing aid in the inner canal without compromising insertion capability at a distal end of the hearing aid.

BRIEF DESCRIPTION OF THE DRAWINGS

The foregoing and other objects, features and advantages of the invention will be

15 apparent from the following more particular description of preferred embodiments of the invention, as illustrated in the accompanying drawings in which like reference characters refer to the same parts throughout the different views. The drawings are not necessarily to scale, emphasis instead being placed upon illustrating the principles of the invention.

20 FIG. 1 is a side view of an embodiment of a half shell of a body for a “one-size-fits-all” “uni-ear” hearing instrument.

FIG. 2 is a perspective view of an embodiment of a complete hearing instrument formed by two half shells of FIG. 1 plus a flexible tip.

FIG. 3 is a cutaway view of an ear showing a detail of a block used in the

25 process of forming an ear impression.

FIG. 4 is a schematic of synchronized scanning method used to generate topological data from ear impressions.

FIG. 5 is a chart of ear canal lengths in mm taken from a number of ear impressions of subjects as measured from the aperture (opening) of the ear canal to the maximum length of the ear impressions.

FIG. 6A is a "frontal" view graph of diameter in mm versus the maximum, mean, and minimum diameter taken from ear impressions of a number of subject's versus various critical points in the ear canal, i.e., at the aperture, after the first bend and near the tympanic membrane.

FIG. 6B is a "top view" as in FIG. 6A.

FIG. 7A is a left ear image shown from the front indicating where the sectional diameters are measured.

FIG. 7B is an image as in FIG. 7 taken from the top.

FIG. 8 is a top view of a uni-ear body 92 showing where the sectional views of FIGs. 9A-M are taken.

FIGs. 9A-9M are various sectional views of FIG. 8.

15 DETAILED DESCRIPTION OF THE INVENTION

A description of preferred embodiments of the invention follows.

The invention will now be described with reference to several embodiments selected for illustration. It will be appreciated that the invention is not limited to the specific embodiments shown in the drawings or described herein. The following description is not intended to limit the scope or spirit of the invention, which is defined separately in the appended claims.

The traditional process of fitting a patient with a hearing instrument involves a fairly long and cumbersome process. This procedure sequentially requires (1) that testing be done to quantify the spectral and intensity characteristics of one's hearing loss, (2) the generation of custom ear impressions for each ear to be fitted with an aid, (3) fabrication of custom hearing instruments using the ear impressions as templates, and (4) possibly the modification of these parts to obtain an acceptable fit. The typical time scale for this entire process is about two weeks. A goal of the present invention is

to eliminate steps (2) through (4) above, so that patients may be fitted with hearing instruments in less than an hour.

To this end, a “one-size-fits-all” peritympanic (deep canal fitting) uni-hearing aid instrument has been developed in accordance with the invention. The primary
5 obstacles impeding these goals were the plethora of shapes, sizes, and curvatures of various ear canals. The present invention provides a hearing instrument that comprises a semi-rigid body shaped so as to accommodate the first (outermost) bend in the ear canal, coupled with a flexible tip capable of traversing the first bend and subsequently, conforming to the second bend. Initially, these requirements result in two shapes; a
10 “one-size-fits-all” unit for either the left ear or right ear. Next, by forming a mirror image of the shape of one of the units, a single shape for a hearing instrument can be generated as described below which will fit in either ear, i.e. a “one-size-fits all” uni-ear device.

In general, the process begins by gathering many (100 or more) ear impressions
15 that are representative of the (target) population. It is not necessary to collect both left and right ear samples since either will suffice. Topological data is then obtained by employing three-dimensional scanning, cross-sectioning, or equivalent methods. The topological data is then transferred to a solid modeling software package so that volumes representing the scanned ear impressions are created. Once the volume
20 dimensions have been properly oriented and aligned, a new volume dimension is created that is the intersection of all the prior dimensions. The single resultant dimension is then truncated and smoothed, and is now suitable for use in one ear only (e.g., either a left-ear or right ear unit).

It was observed that the single-ear units created in the manner detailed above
25 exhibit a considerable amount of mirror symmetry. In fact, this symmetry is lost only at that distal end of the hearing aid near the outer region of the ear canal. Thus, to obtain a uni-ear device, it was determined that one could (using solid modeling software) create a mirror image of the single left or right hearing instrument body and then align and intersect these two bodies, i.e., the original and the mirror image dimensions. These

two entities were found to have a relatively large overlap. After some minor smoothing (used to minimize the visual impact) and radiusing operations, the set of volume dimensions that results from the prior intersection may be used to contain a uni-ear device when coupled with a flexible distal tip to fit deeply into the ear canal.

5 A method for fabricating hearing aid bodies having the desired shape is to produce two semi-rigid half shells 110, one of which is shown in Fig. 1. Joining the shells results in a single rigid body 100 as shown in the perspective of FIG. 2. Note that this shell 10 has features that are adapted to contain internal components such as a microphone, battery, and a receiver, etc. (not shown). In one embodiment, the shell
10 may contain a permanently wired-in battery as disclosed in copending patent application Serial No. 09/263,593, filed March 5, 1999 entitled "Disposable Hearing Aid with Integral Power Source" (incorporated herein in its entirety by reference) such that the hearing aid is not readily repairable, rather it is intended to be disposable after its useful life. Another important pertinent attribute of the finished shell is that it is shaped to fit
15 either ear for most people. The body 100, as shown in FIG. 2, of the hearing instrument is also adapted to hold a soft tip 12 at a relative angle to enhance retention of the unit in the ear without compromising insertion.

The following sections outline one possible procedure for making a mold for a "uni-ear" device.

20 1. Ear Inspection

The first step is to collect a plurality of ear impressions of a representative target population. Before making an impression the ear should be inspected. To properly inspect the ear, the pinna is grasped between the thumb and index finger and gently pulled back and slightly up. This action straightens the canal to facilitate the placement
25 of an otoscope into the canal. In working with children, it is generally suggested that the pinna be pulled slightly down and back.

The ear is inspected for any discharging condition. If there is any discharge in the ear, the person inspected should be seen by an ear physician, and no ear impression

should be made. Also, inspect for irregularities in the canal, foreign objects, or for any other contraindications, including excessive cerumen. If there is an obstruction, the person should be referred to a physician. To assure a good impression, note the following: (1) size of canal - to determine the size of the ear impression, (2) the texture of ear and canal - with very soft ears, it is easy to distort the impression when putting the material into the canal and ear, (3) angle and direction of canal - it is important that the impression is a true and complete picture of the ear canal, (4) canal length - the canal of the ear impression must be long enough to direct sound to the eardrum (this would be past the second directional turn).

10 2. Preparing the Canal

Before injecting the impression material into the canal, a block 20 must be inserted to a location proximal to the tympanic membrane as depicted in FIG. 3. A foam block or cotton block 20 of the proper size as determined from the ear inspection should be used. Be sure that a thread or dental floss 22 is securely attached to the block.

- 15 Insert the block into the canal. It is generally a good idea to guide the block into the canal with an ear light. Always support the hand with the ear light to prevent any injury if there should be any rapid head movement. Insert the block to a sufficient depth to allow the impression to include the second directional bend in order to direct the sound to the tympanic membrane. An ear block 20 is required for making all impressions as it
- 20 (1) protects the eardrum from damage, (2) blocks material and allows it to expand to fill the whole canal, and (3) assures a complete canal with the proper final bend. In some instances, it may be necessary to trim excessive hair in the canal. Be sure to use blunt tipped scissors to reduce the possibility of injury to the ear.

3. Making the Impressions

- 25 1. Always prepare the materials in advance.
2. Follow the mixing instructions for the material in use.

3. With powder-liquid materials, mix with a spatula until a smooth creamy consistency is reached and the material has begun to congeal. With solid materials, knead equal amounts of both components until colors are evenly blended.
- 5 4. Working rapidly, place the material in the proper syringe. Press the plunger forward until a small amount of material is ejected.
5. With the canal block 20 in the ear, place the nozzle tip of the syringe in the opening to the ear canal. Be sure to support your hand to avoid any injury in the event of any rapid heard movement. Press the plunger gently, gradually withdrawing the syringe as the material fills the canal and begins to flow out into the concha and helix areas. Be sure to fill the entire outer ear, especially the helix area, and keep the nozzle submerged in the material at all times for better filling and completeness of the total impression.
- 10 6. After the canal and outer ear are completely filled, apply only slight pressure on the outer surface of the impression to smooth for mailing purposes.
- 15 7. Allow sufficient time for the impression to set. Ten minutes is the minimum time recommended. Check by making an indention with the thumb nail. If properly set up, no mark should remain.
- 20 8. Gently break the seal at as many points as possible to prevent distortion and reduce stress when removing the impression.
9. Grasp the pinna firmly with one hand the impression with the other, rotate it slowly with an upward and outward motion. The canal block should remain an integral part of the impression.
- 25 10. Reinspect the canal with an otoscope after removal to be sure the ear is clear.

4. Examining the Impressions

After removal of the impression, critically evaluate all areas for accuracy. If the impression does not represent a true picture of the ear, the best time to make a second impression is now. In the long run, it will save time in modifications and remakes.

5 5. Generating Topological Data from the Ear Impressions Using 3D Scanning

3D scanning of the ear impressions are implemented as follows:

Synchronized scanning geometry, based on a doubled-sided mirror (used to project and detect a focused or collimated laser beam) as shown in FIG. 4 is used for this purpose. A light source such as a laser 24 is coupled to an optical fiber 26. A scanning mirror 30 and fixed mirrors 32, 34 are used to project the laser beam 38 on the impression 40. The scattered light is collected through the same scanning mirror 30 and projected and focused by lens 42 onto a linear CCD array 44. Note that the CCD 44 is tilted to compensate for defocusing at the detection site. With careful optical design, the divergence of the laser beam can be made to match the resolving element field of view of the CCD linear array 44. In such conditions, the parameters of the focused laser beam are kept constant over a large depth of view. This enables 3-D digitizing of the impressions 40 from a very short distance (10's of cm) to a large distance (10 meters) without refocusing or processing algorithm modifications. The configuration illustrated in FIG. 4 is a profile measurement device. A second scanning mirror (not shown) is used to deflect orthogonally both the projected and the reflected laser light. The whole arrangement can be mechanically translated by commercially available gantry linear positioning device or by rotary table. A typical large field of view 3-D laser scanner uses two orthogonal galvonometers to address a 4000 pixel by 4000 pixel field of view. This optical configuration allows 3-D recordings from 50cm to 10m from the scanner using a linear CCD array as a position sensor. The minimum element of resolution of the CCD corresponds to a resolution in depth of 100 microns at 50cm, and approximately increases as the square of the distance.

An alternative relatively inexpensive method for obtaining 3D scans of ear impressions utilizes cameras. For example, 3Scan (from Geometrix, Inc.) can be used to replace the expensive laser scanning hardware of FIG. 4 with a low-cost digital camera. The computer-controlled camera takes multiple images of an object rotating on a computer-controlled turntable. From these images, 3Scan software extracts the complete 3D geometry of the object and maps textures from the original imagery onto the geometry. User-selectable polygon decimation supports the output of model complexities from 100 polygons to 1,000,000 polygons in a variety of industry standard file formats.

6. Transferring the Data into the Solid Modeling Software

The scanning tools described above generate data representing the shape of the surfaces of many ear impressions that have been scanned. This information is called "cloud point" data. This cloud point data is subsequently "read" into a software package such as "Pro Surface" from Parametric Technologies, Inc.

7. Properly Aligning and Orienting Volumes

Once the "cloud point" data has been transferred into "Pro/Surface", the space enclosed by the surfaces is converted into volumes using "Pro/Engineer". For each part scanned, separate volumes are created in this manner. Using the assembly mode of Pro/Engineer, each volume/part is placed in the assembly so as to maximize the overlapped regions.

8. Creating a New Volume that is the Intersection of the Prior Volumes

When all of the volumes have been (positioned) to maximize the overlap, Boolean operations are used to calculate a single volume resulting from the intersection of all other volumes. A software package that can be used to perform the necessary Boolean operations is the ANSYS finite element software.

9. Truncating and Smoothing the Resultant Volume

Next, a software package such as Pro/Engineer is used to truncate and smooth the resultant volume using cuts, radii, and other features until a desirable “one-size-fits-all” shape is obtained which will fit into one side of most ears.

5 10. Create Uni-Ear Part

The part generated so far would be suitable for one ear only. However, using this part, a mirror image model thereof is generated, again using a program such as Pro/Engineer. This provides mathematical models of two volumes, the original and its mirror image from which a “uni-ear” part can be derived. Once again, using the
10 assembly mode of Pro/Engineer, these two volumes are placed in a new assembly so as to again maximize the overlapped regions. When all of the volumes have been properly positioned, boolean operations, as before, are utilized to calculate a single volume resulting from the intersection of these two volumes.

11. The single volume is then used to create two hollow half-shells having a composite
15 shape in the form of such volume. The two shells when bonded together house the components needed for a functional hearing aid and retain at a distal end a flexible tip with a hollow sound tube which extends toward the tympanic membrane when the hearing aid is inserted into the ear canal.

While this invention has been particularly shown and described with references
20 to preferred embodiments thereof, it will be understood by those skilled in the art that various changes in form and details may be made therein without departing from the scope of the invention encompassed by the appended claims. For example, an alternate method of making a “one-size-fits-all” uni-hearing aid body is to measure the canal length and cross-sections of the ear canal at certain critical areas, such as, at the
25 aperture, after the first bend and near the tympanic membrane of a number of impressions taken from subjects; as shown in FIGs. 5, 6A and 6B, respectively. These measurements are then used to create cross-sectional maximum, mean, and minimum

CLAIMS

What is claimed is:

1. A hearing aid body adapted to interchangeably fit inside either a right side or left side of an ear canal of a typical user such that a distal end of the body is
5 disposed proximally adjacent to a tympanic membrane of said user.
2. The body of Claim 1 formed of two half shells joined together with hollow interiors for housing hearing aid components.
3. The body of Claim 2 in which a soft tip is secured at the distal end of the body.
4. The body of Claim 3 wherein the tip includes a sound port for coupling sound
10 from a receiver housed in the body to the membrane of a hearing aid user.
5. A non-specific removable hearing aid having a shell which is shaped to be useable with a right ear or left ear and which houses the requisite component for a functional hearing aid.
6. The hearing aid of Claim 5 in which the shell is formed of two halves which are
15 bonded together and wherein a flexible tip is retained at a distal end of the shell.
7. The hearing aid of Claim 6 in which the components include a permanently wired battery and the hearing aid is adapted to be disposable.
8. A hearing aid formed of a semi-rigid shell enclosing hearing aid components with a flexible tip retained at one of the shell, the shell having a shape adapted to
20 fit in the ear canal of either a right or left human ear.

9. The hearing aid of Claim 8 in which the tip contains a receiver and a sound tube extending between the receiver and a distal end of the tip.
10. The hearing aid of Claim 9 in which the shell is formed of two half-shells joined together and in which the components include a microphone, and signal
5 processing electronics and a battery permanently wired to the electronics.
11. A method of making a model of a hearing aid housing which is adapted to be inserted into either a right side or a left side of an ear canal adjacent to a tympanic membrane of a typical user comprising the steps of:
- 10 a) obtaining sample ear impressions from a plurality of subjects;
b) generating three-dimensional topological data corresponding to each the surface of the samples;
c) generating volume data representing volumes corresponding to the 3D geometry of the topological data obtained from each sample;
processing the volume data of each sample to generate a first single set
15 of data which represents the intersection of all the volumes;
e) using the first set of data to generate a second set of data representing a mirror image of the first set of data;
f) using the first and second sets of data to generate a third set of data representing a third volume resulting from the intersection of the two sets of
20 data; and
g) using the third set of data to produce a physical model representing the third volume.
12. A shell for a hearing aid made in accordance with the model made in accordance with the method of Claim 11.
- 25 13. The shell of Claim 12 formed of two half-shells joined together.

14. A hearing aid made from components mounted in the shell of Claim 13.
15. The hearing aid of Claim 14 in which the shell contains at least the following components required for a functional hearing aid, a battery, a microphone, signal processing electronics and a receiver.
16. A body for a hearing aid unit having an oval cross section which gradually varies from an outer dimension of about .519 mm by .406 mm to a middle dimension of about .470 mm by .336 mm and to an inner dimension of about .228 mm by .214 mm.

A one-size-fits-all uni-hearing aid is described which is adapted to fit into either ear of an ear canal of a user to a depth proximal to the tympanic membrane. The hearing aid is comprised of two half shells joined together to house the hearing aid components. The joined shells secure a flexible tip at the distal end of the shell.

Figure 1 shows the results of the first two experiments. The first experiment was designed to test the hypothesis that the effect of the number of stimuli on the response time is a function of the number of stimuli. The results show that the response time increases as the number of stimuli increases, and that the effect of the number of stimuli is a function of the number of stimuli. The second experiment was designed to test the hypothesis that the effect of the number of stimuli on the response time is a function of the number of stimuli. The results show that the response time increases as the number of stimuli increases, and that the effect of the number of stimuli is a function of the number of stimuli.


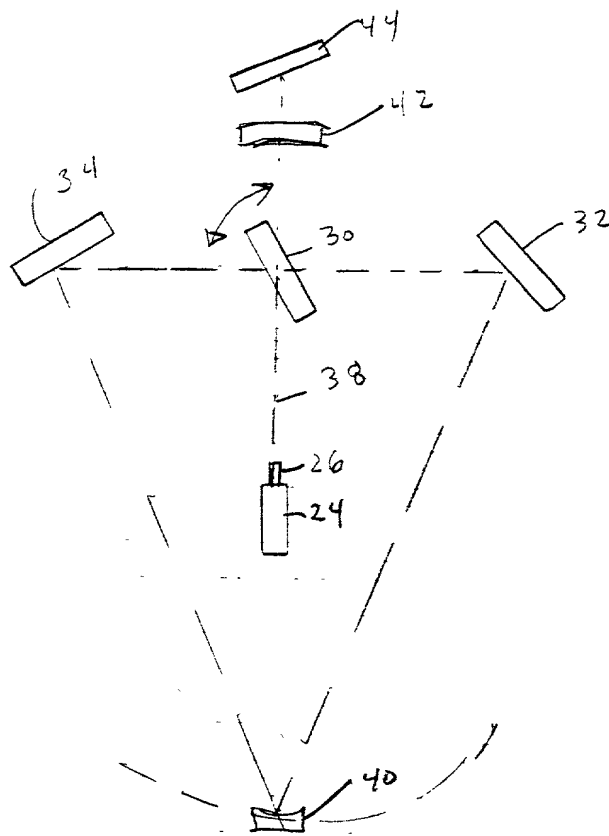


FIG 4

Range = 23 mm to 34 mm
Mean = 28.29 mm

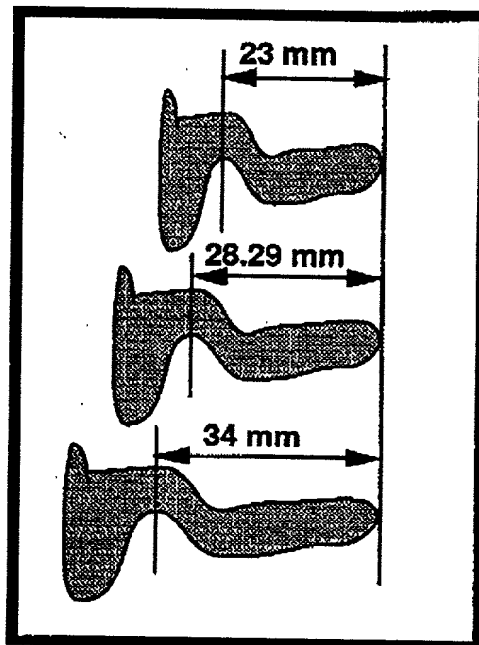

(Top looking down)

Average = 28.29 mm

Left Right
Length in mm as indicated
in drawing below

33	28
31	30
26	28
30	23
27	33
26	27
27	29
27	27
26	31
25	26
30	30
30	25
26	28
26	29
33	34
30	29
	26
	30
	27
	25
	28
	29

Average: Left Ear Right Ear
28.31 mm 28.27 mm

FIG-5

(Frontal View)

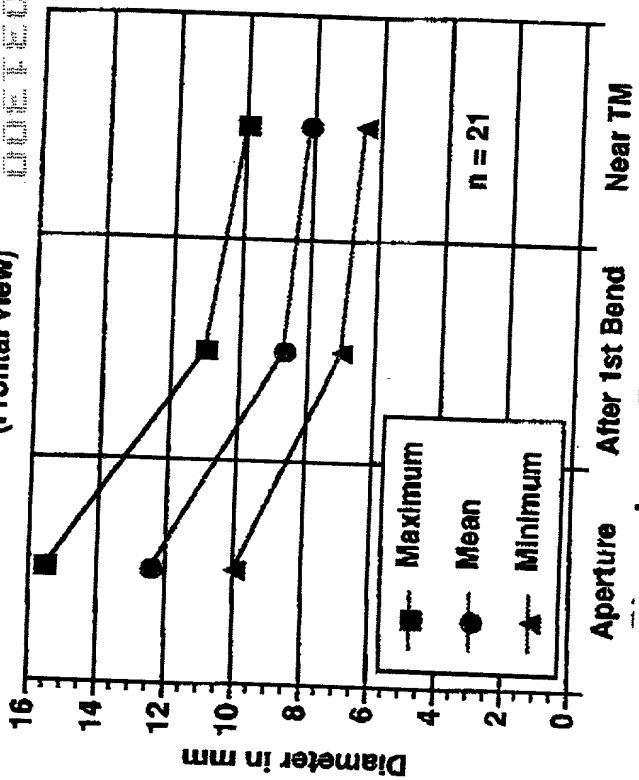


FIG 6A

(Top View)

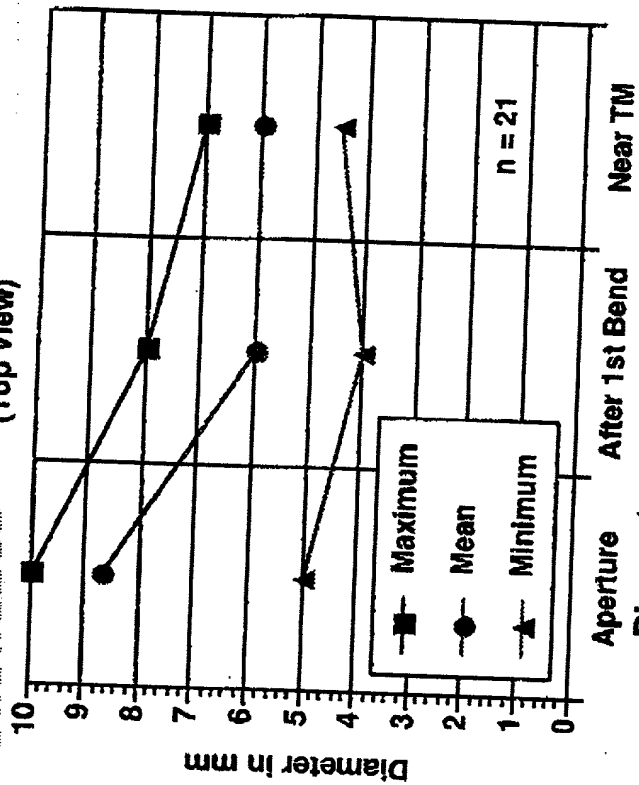


FIG 6B

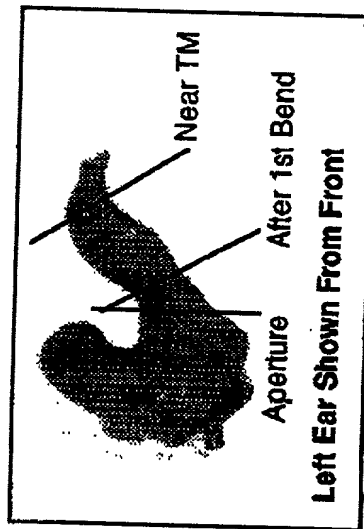


FIG 7A


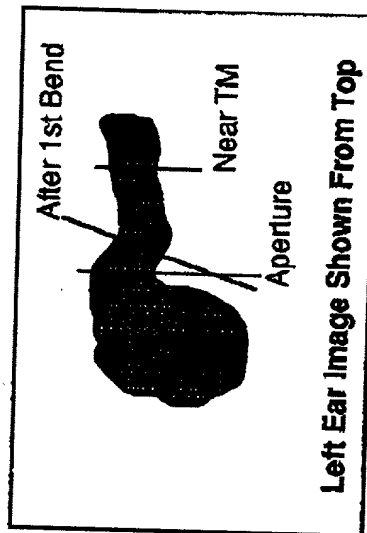


FIG 7B

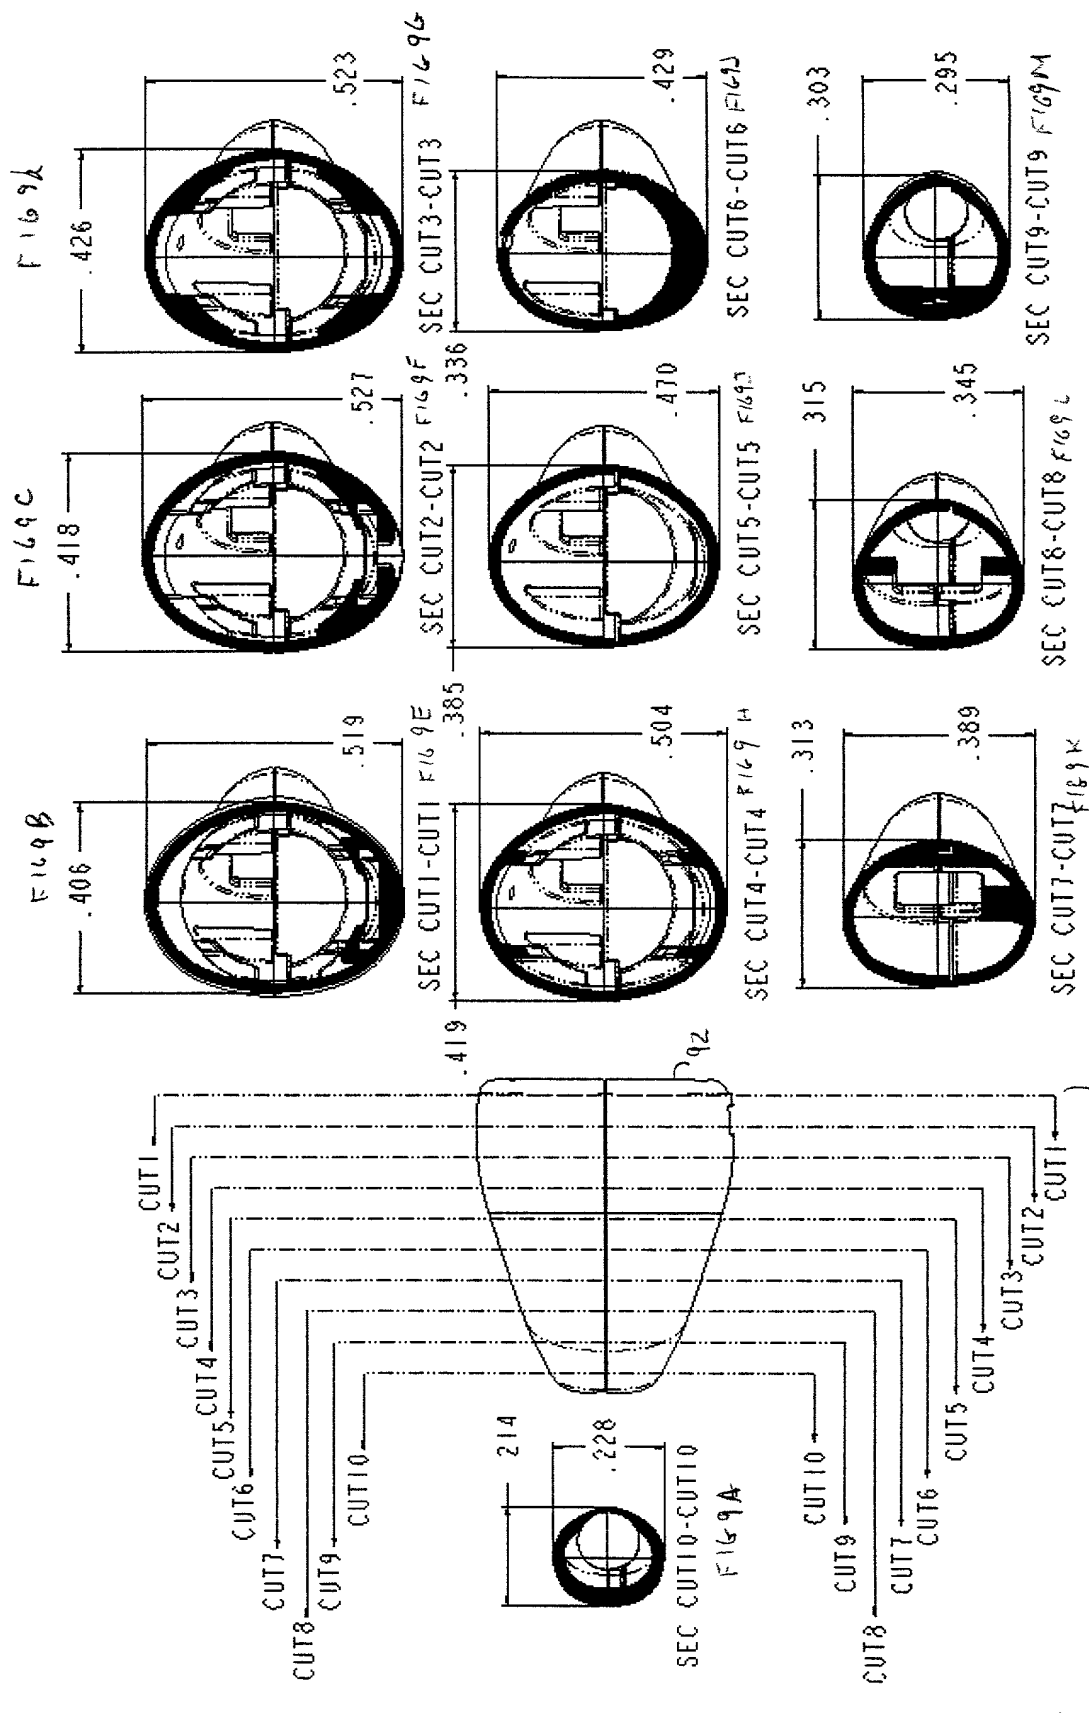

168